

TEST REPORT

(Electronic version)



No: 200084822

VERIFICATION WEBSITE: www.gttc.net.cn

VERIFICATION CODE: YRCG-2411-54

ISSUE DATE 签发日期: 2020-04-28

扫码下载报告



APPLICANT: ZHENGZHOU YLW TECHNOLOGY CO., LTD

委托单位: 亚利韦(郑州)科技有限公司

ADDRESS: LINYUAN INDUSTRIAL PARK, YANHE ROAD, HEZHUANG TOWN, XINZHENG CITY, HENAN, CHINA

地址: 新郑市和庄镇神州路沿河路交叉口东150米林源工业园区

INFORMATION CONFIRMED BY APPLICANT 客户认定信息:

DISPOSABLE RESPIRATOR MASK 防颗粒物呼吸器口罩 30个

COLOUR 颜色: 白色

MANUFACTURE'S NAME 生产单位: 亚利韦(郑州)科技有限公司

DATE RECEIVED/DATE TEST STARTED: 2020-04-20

样品受理/测试开始日期: 2020-04-20

CONCLUSION 结论:

VISUAL FIELD 视野	M
FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER NaCl颗粒物过滤效率	M
INSPIRATORY RESISTANCE 吸气阻力	M
EXPIRATORY RESISTANCE 呼气阻力	M
FLAMMABILITY 可燃性	M
HEAD BAND 头带	M
APPEARANCE INSPECTION[2 PIECES] 外观检查[2个]	M

APPROVED BY(签发):

郭子山 高级工程师

ZiShan Guo SENIOR ENGINEER

郭子山



TEST REPORT

(Electronic version)



No: 200084822

VERIFICATION WEBSITE: www.gttc.net.cn

VERIFICATION CODE: YRCG-2411-54

ISSUE DATE 签发日期: 2020-04-28

扫码下载报告



NOTE: “M” -MEET THE STANDARD’S REQUIREMENT “F” -FAIL TO MEET THE STANDARD’S REQUIREMENT
“---” -NO COMMENT
备注: “M” -符合标准要求 “F” -不符合标准要求
“---” -此项目不判定

REMARK:

THE AUTHORIZATION OF APPEARANCE INSPECTION IS NOT RECEIVED FROM CNAS.

外观检查项目暂未获得CNAS认可。

ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).

本报告中检验检测项目均在相应标准规定的环境条件下进行（有注明的除外）。

COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.

复印件、副本未重新加盖报告书确认章无效。

THE EXPERIMENT WAS CARRIED OUT AT No.1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

本报告检验检测地址为广州市番禺区珠江路1号。

APPROVED BY (签发):

郭子山 高级工程师

ZiShan Guo SENIOR ENGINEER


郭子山



TEST REPORT

(Electronic version)

No:200084822

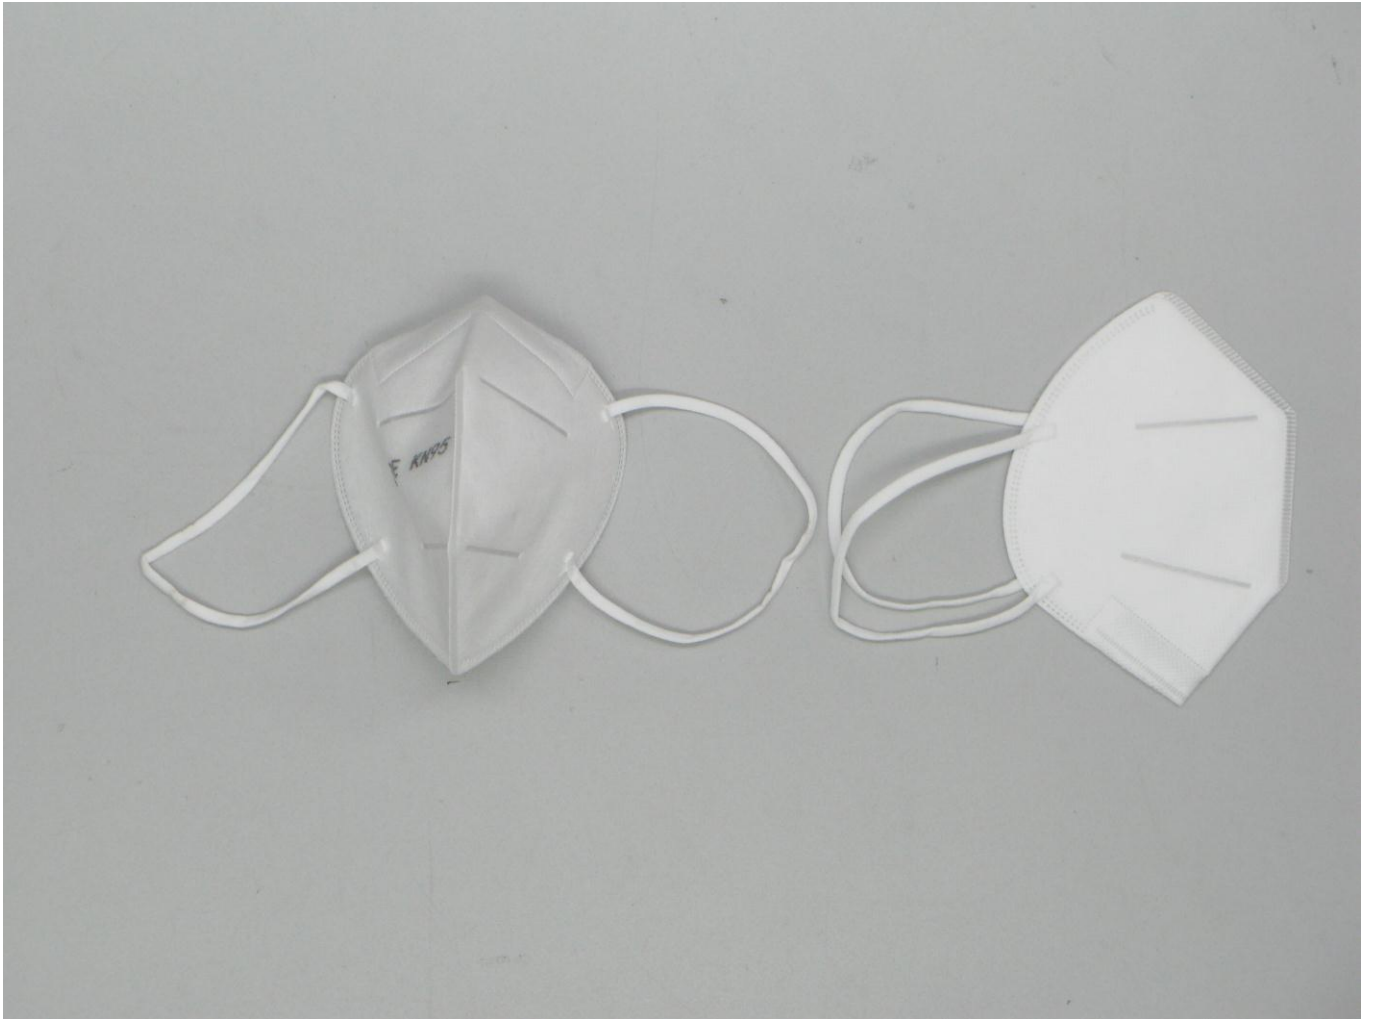

TEST REPORT

(Electronic version)

No:200084822

VISUAL FIELD(°)
视野(°)

(GB 2890-2009 6.8)

70

REQUIREMENT 要求
≥60
(GB 2626-2006)

FILTRATION EFFICIENCY TO NaCl PARTICULATE MATTER

NaCl颗粒物过滤效率

(GB 2626-2006 6.3, AIR FLOW 空气流量:85L/min, AEROSOL 气溶胶颗粒:NaCl, AEROSOL CONCENTRATION 气溶胶浓度, 15mg/m³, TEMP 温度:23.8℃ RH 湿度:34.6%)

FILTRATION EFFICIENCY 过滤效率(%) :

UNTREATED SAMPLE 未处理样品

1# 98.75
2# 98.16
3# 98.70
4# 98.54
5# 97.96
6# 98.25
7# 98.41
8# 97.88
9# 98.29
10# 98.47

REQUIREMENT 要求

FILTRATION EFFICIENCY 过滤效率(%) :

≥95.0
(KN95)
(GB 2626-2006)

CONDITIONING TREATED 温湿度预处理后样品

1# 96.86
2# 96.53
3# 96.74
4# 97.12
5# 96.81

INSPIRATORY RESISTANCE (Pa)

吸气阻力(Pa)

(GB 2626-2006 6.5, HEAD SIZE 头模: MEDIUM 中号)

UNTREATED SAMPLE 未处理样品:

1# 64.8
2# 68.4

REQUIREMENT 要求

≤350
(GB 2626-2006)

PRETREATMENT SAMPLE 预处理样品:

1# 79.2
2# 75.8

EXPIRATORY RESISTANCE (Pa)

呼气阻力(Pa)

(GB 2626-2006 6.6, HEAD SIZE 头模: MEDIUM 中号)

UNTREATED SAMPLE 未处理样品:

1# 62.3
2# 60.3

REQUIREMENT 要求

≤250
(GB 2626-2006)

PRETREATMENT SAMPLE 预处理样品:

1# 65.3
2# 64.2



PAGE 4 OF 5

TEST REPORT

(Electronic version)

No:200084822

FLAMMABILITY(s) 可燃性(s)

(GB 2626-2006 6.15)

AFTERFLAME TIME 续燃时间
UNTREATED SAMPLE 未处理样品

1# 0.0
2# 0.0

CONDITIONING TREATED 温湿度预处理后样品

3# 0.0
4# 0.0

REQUIREMENT 要求

AFTERFLAME TIME 续燃时间

≤5
(GB 2626-2006)

HEAD BAND 头带

(GB 2626-2006 6.11)

UNTREATED SAMPLE 未处理样品:

1# PASS 符合要求

CONDITIONING TREATED 温湿度预处理后样品:

1# PASS 符合要求

REQUIREMENT 要求

EACH HEAD BAND, BUCKLE AND OTHER ADJUST
PARTS OF MASK SHOULD NOT SLIP OR BREAK
UNDER 10N TENSION FOR 10S.

面罩的每条头带、带扣及其他调节部件在承受
10N的拉力,持续10s,不应出现滑脱或断裂。
(GB 2626-2006)

APPEARANCE INSPECTION[2 PIECES] 外观检查[2个]

(GB 2626-2006 6.1)

PASS
符合要求

REQUIREMENT 要求

ACCORDING TO THE CLAUSE 5.2 OF THE
PRODUCT STANDARD

按标准5.2条要求
(GB 2626-2006)



——本报告结束(End of Report)——

PAGE 5 OF 5